


5973 Air and Water Check

Instrument: MSD22

Sun Jul 23 10:12:58 2006

C:\MSDCHEM\1\5973N\

Scan: 10.00 - 75.00 Samples: 8 Thresh: 0 Step: 0.10
69 peaks Base: 69.00 Abundance: 322304

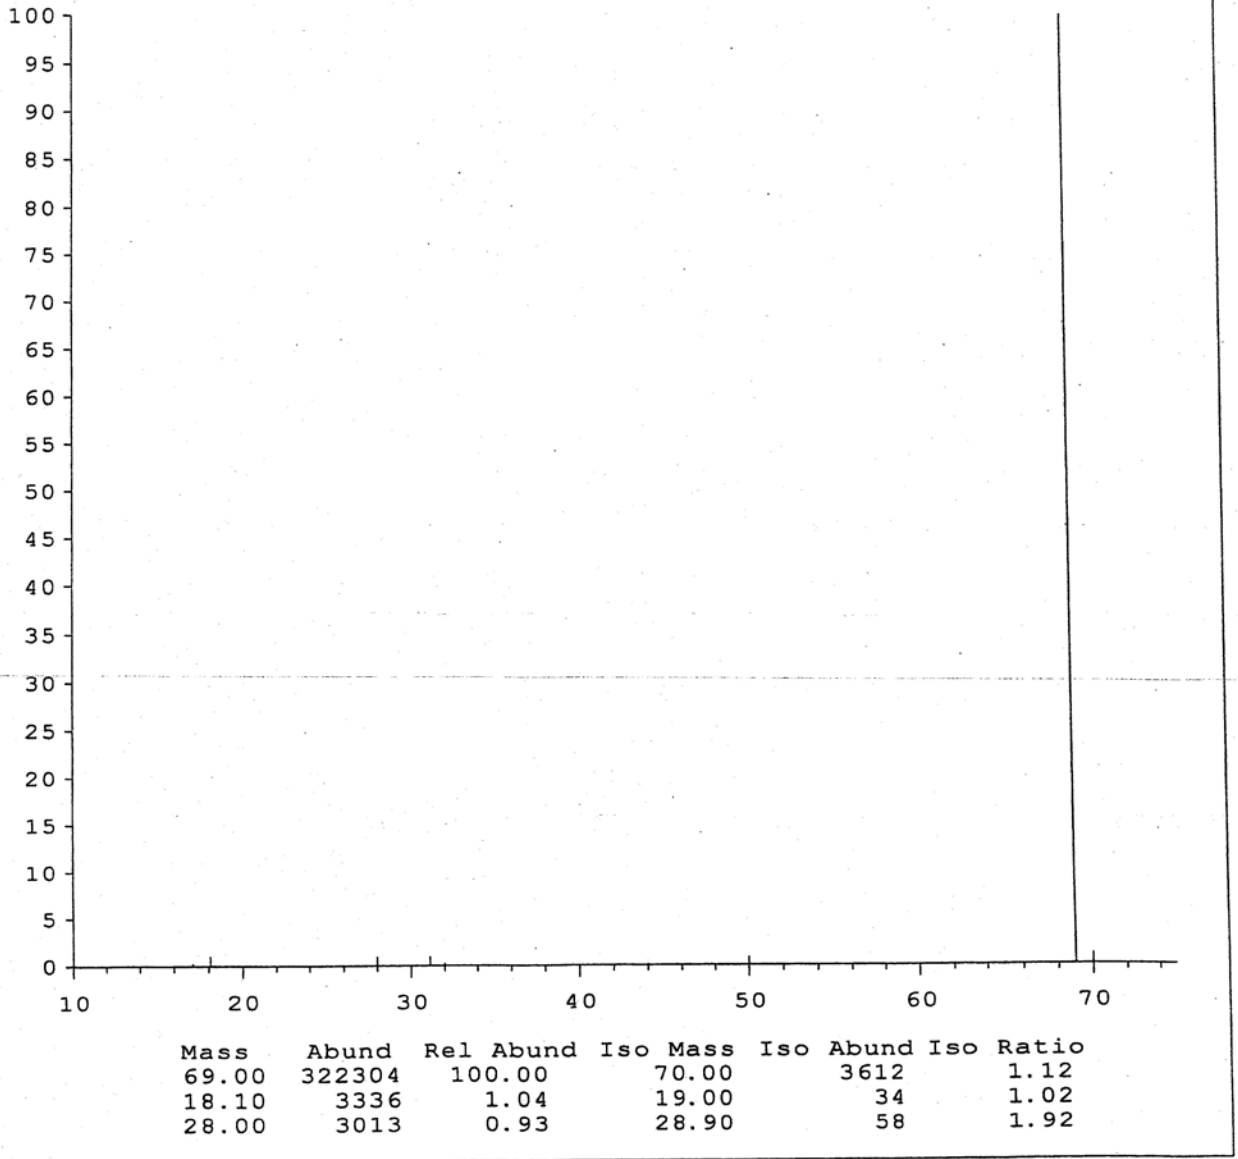

Current Params used: ATUNE.U

Relative abundances:

18/69 = 1.04	Water%
28/69 = 0.93	Nitrogen%
32/69 = 0.28	Oxygen%
44/69 = 0.17	Carbon Dioxide%
28/18 = 90.32	Nitrogen/Water%